

SNC Patient QA of Dose Distribution

Hospital

[REDACTED]

QA Date

26 Nov 2020 12:21:27



QA Parameters

Patient Name

[REDACTED]

Patient ID

[REDACTED]

Plan Name

qa2

Plan ID

[REDACTED]

Plan Date

04 Apr 2019 16:31:58

Verified Plan UID

[REDACTED]

Total MU

675.5

Absolute Dose Comparison (GC/Gamma using 3D Mode)

Threshold (%)	20.0	Use Global (%)	No
Difference (%)	2.0	Meas Uncertainty	No
Distance (mm)	2	Cavity Dose	N/A

Summary (GC Analysis)

Pass (%)	91.3
Pass	454
Fail	43
Total Points	497

Dose Values in cGy

	CAX	Norm	Sel	Max
Set 1		82.81	47.22	89.08
Set 2	48.41	88.19	50.53	92.35
Set 1-2		-5.38	-3.32	-3.26
% Diff		-6.10	-6.56	-3.53
DTA(mm)	N/A	N/A	N/A	


Notes

bst2

Reviewed By

Physics

ArcCHECK (Set 1)

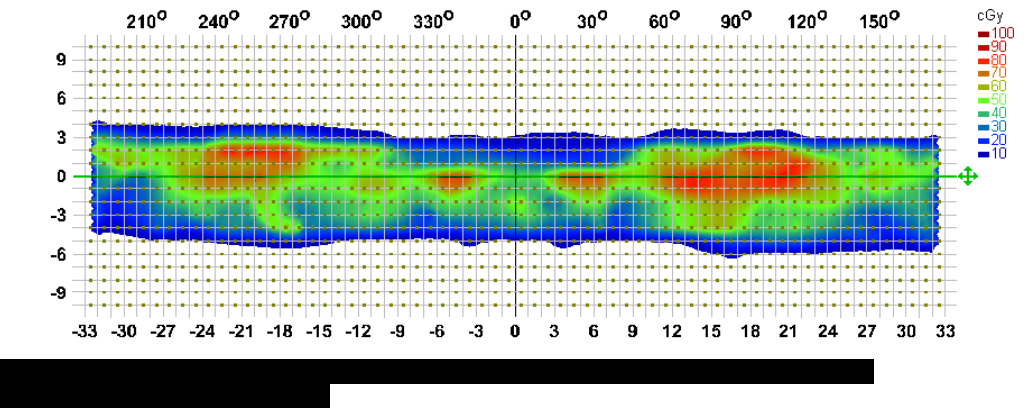


CAX Coords (x,y) (mm)
0, 0

Norm Coords (x,y) (mm)
215.00, 10.00

SEL Coords (x,y) (mm)
-5.00, 0.00

Plan (Set 2)

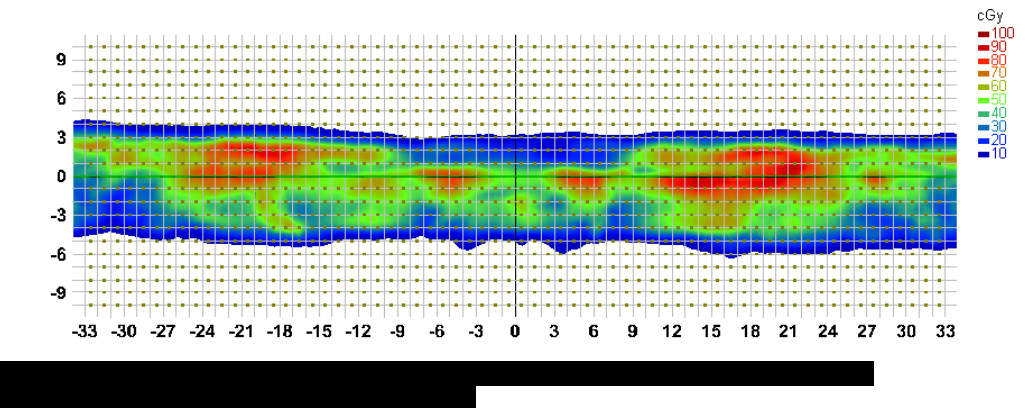

CAX Coords (x,y) (mm)
0, 0


Norm Coords (x,y) (mm)
215.00, 10.00

CAX Offset (x,y) mm
0, 0

Dose Scaling Factor
1.0

Isocenter Coords (x,y,z) (mm)
0.000, 0.000, 0.000

ArcCHECK - Plan (Set 1-2)

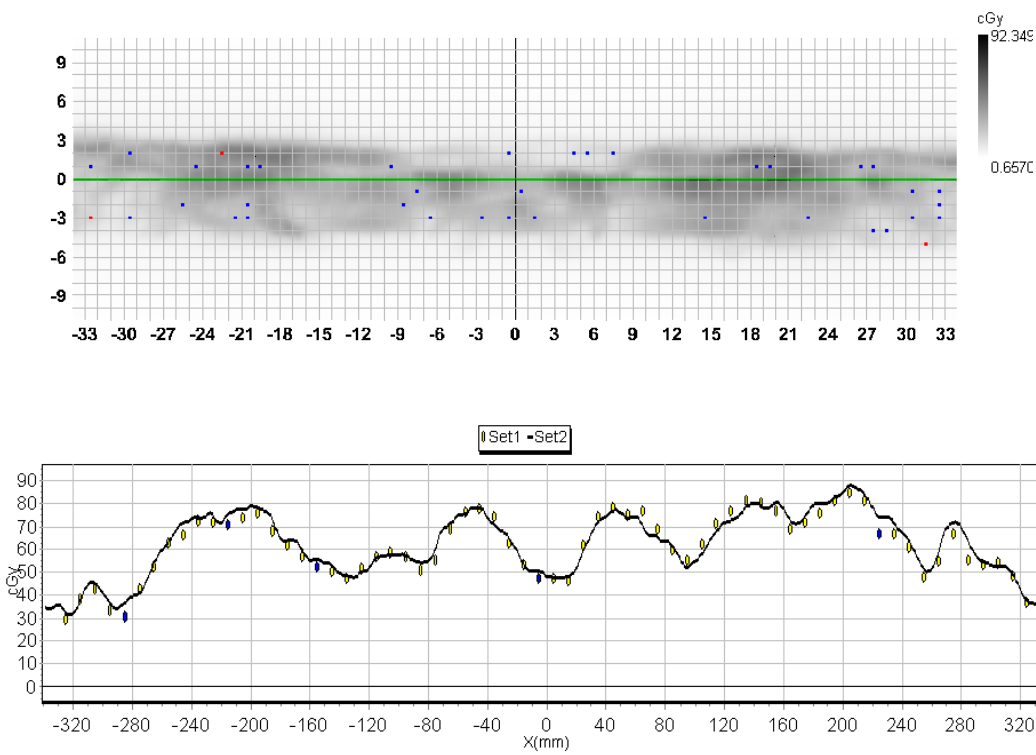

Gamma Index Summary

	Min	Max
Points In Threshold	N/A	N/A
All Points	N/A	N/A
	Average	Stdv
Points In Threshold	N/A	N/A
All Points	N/A	N/A